

Nitrogen Dioxide Tube Instructions

Shelf life: This tube has a shelf life of 12 weeks. Tubes must be exposed and returned for analysis within this period.

Tube storage: Tubes should be refrigerated before exposure and should not be subject to large variations in ambient temperature. Do not exceed the shelf life. If using blank tubes, do not remove the tube from the packaging. Store both tubes in the same conditions as the sampling tubes.

Fixing tubes: It is important that the end of the tube is in an area with a free circulation of air. Certain surfaces may act as absorbers leading to reduced atmospheric concentrations immediately adjacent to the tube. For this reason tubes should not be mounted directly onto a surface. Ideally a spacer of at least 5cm should be used between the surface and the tube. The spacer should not be placed in any form of recess (to avoid the possibility of sampling stagnant air). To avoid sampling in an area of higher than usual turbulence, tubes should not be located on the corner of a building.

Exposure:



1. Remove WHITE cap from the tube. Keep cap in a safe place.
2. Position each tube vertically with the open end facing downwards during required sampling period (2-4 weeks).
3. After sampling, replace the WHITE cap on the tube. **Label the tube and the exposure sheet clearly with the supplied barcode labels (see below).**

Returning tubes: Tubes should be returned as soon as possible after exposure. Fill in exposure sheet including exposure time. Tubes should be returned in a sealed container, such as the plastic bag that they are received in.

Return address:

Ormantine USA Ltd. Inc. 1740 Convair Street Palm Bay, FL 32909
Tel: +1 (321) 676-7003
Email: diffusion@ormenviro.com

New Barcoding for Tubes


On receiving your delivery, you should find enclosed

- A copy of an exposure sheet
- A strip of bar codes
- Your tubes




We recommend that you label your tubes (and sheets) at the point of placing the tubes on site.

Simply take the 1st of the duplicate labels (1.) and stick it to the appropriate location on the exposure sheet (2.).

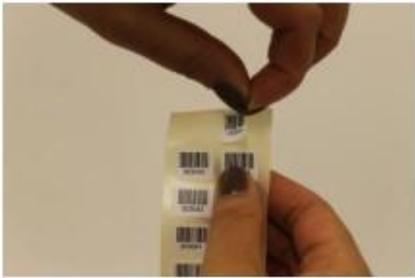

1.

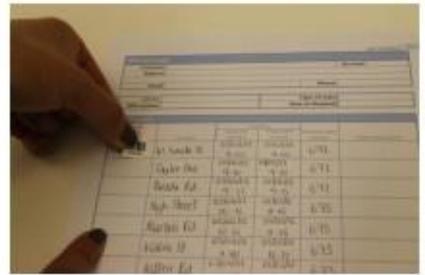

2.

Then take the 2nd matching label (3.) and stick it to the tube exposed at the same location (4.).

Please take care to make sure the label is securely fixed to the tube (5.).
These labels are treated to deal with the weather conditions.



3.



4.



5.